


Tue Feb 24 08:47:26 2004


TIDE Mass_0

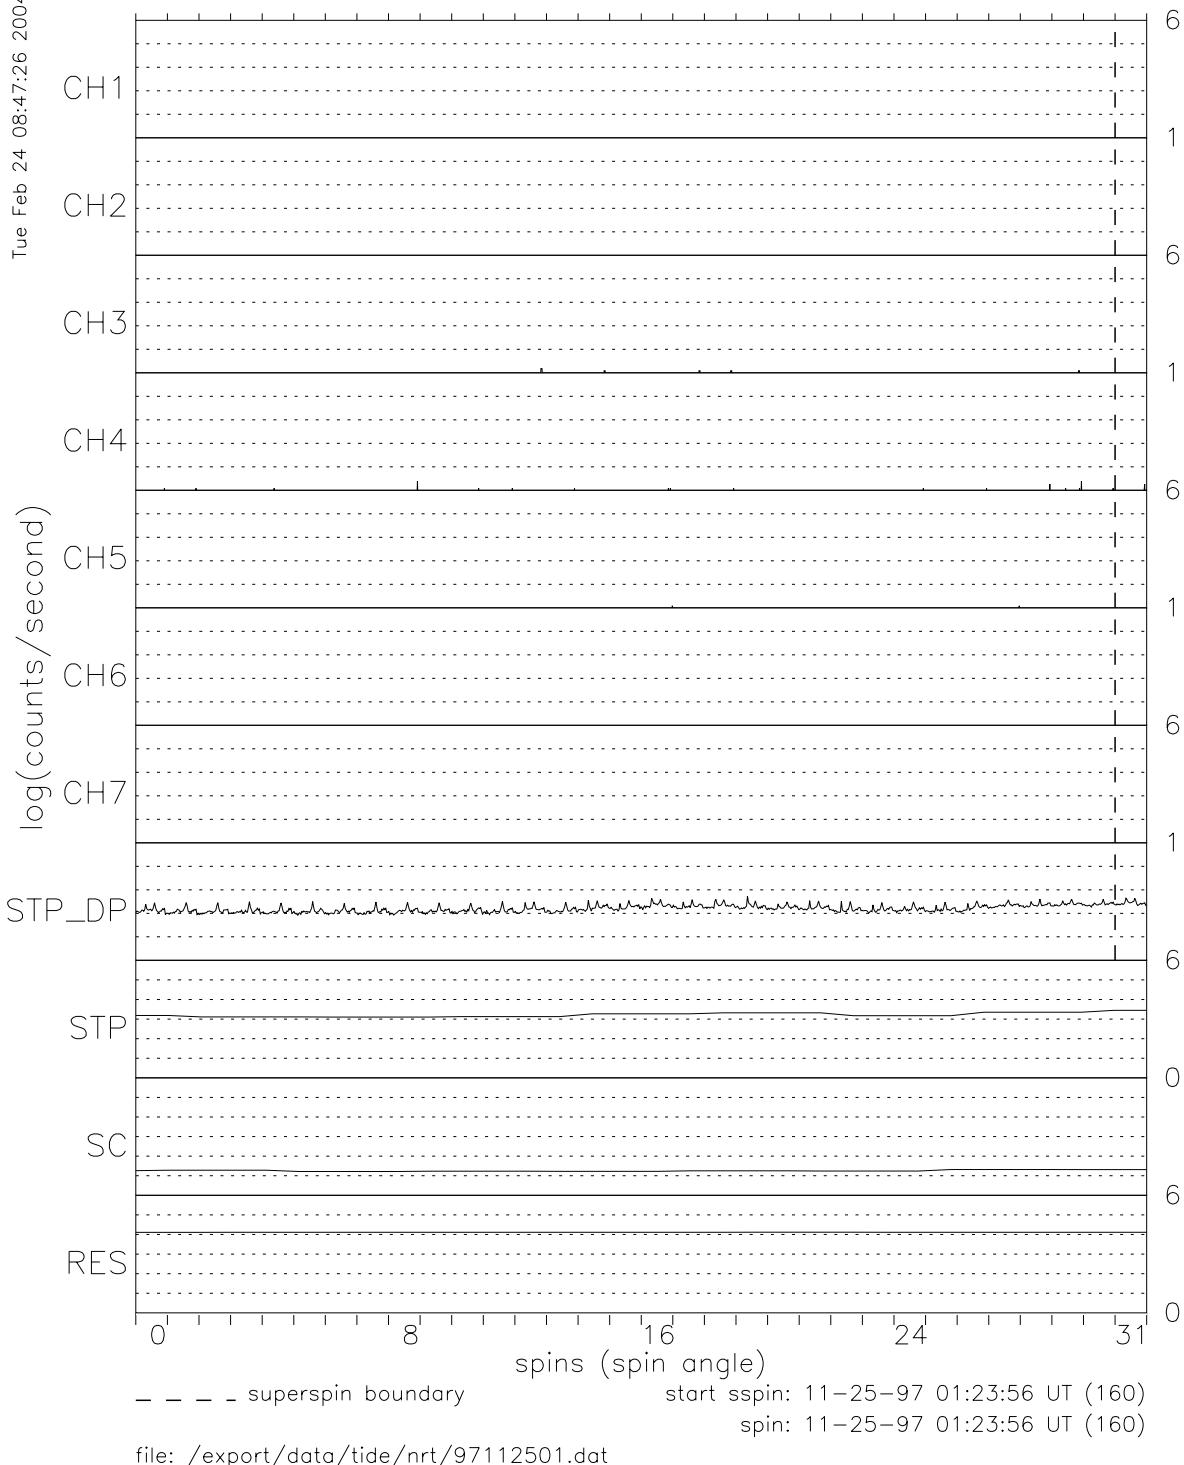

-15kV TOF: -9245 v
-3.6kV MCP: -2593 v
-2.4kV MCP: -1579 v
Input Cur: 294 ma
RPA max: 237 v
Mirror max: 238 v

Tue Feb 24 08:47:26 2004

TIDE Direct Events

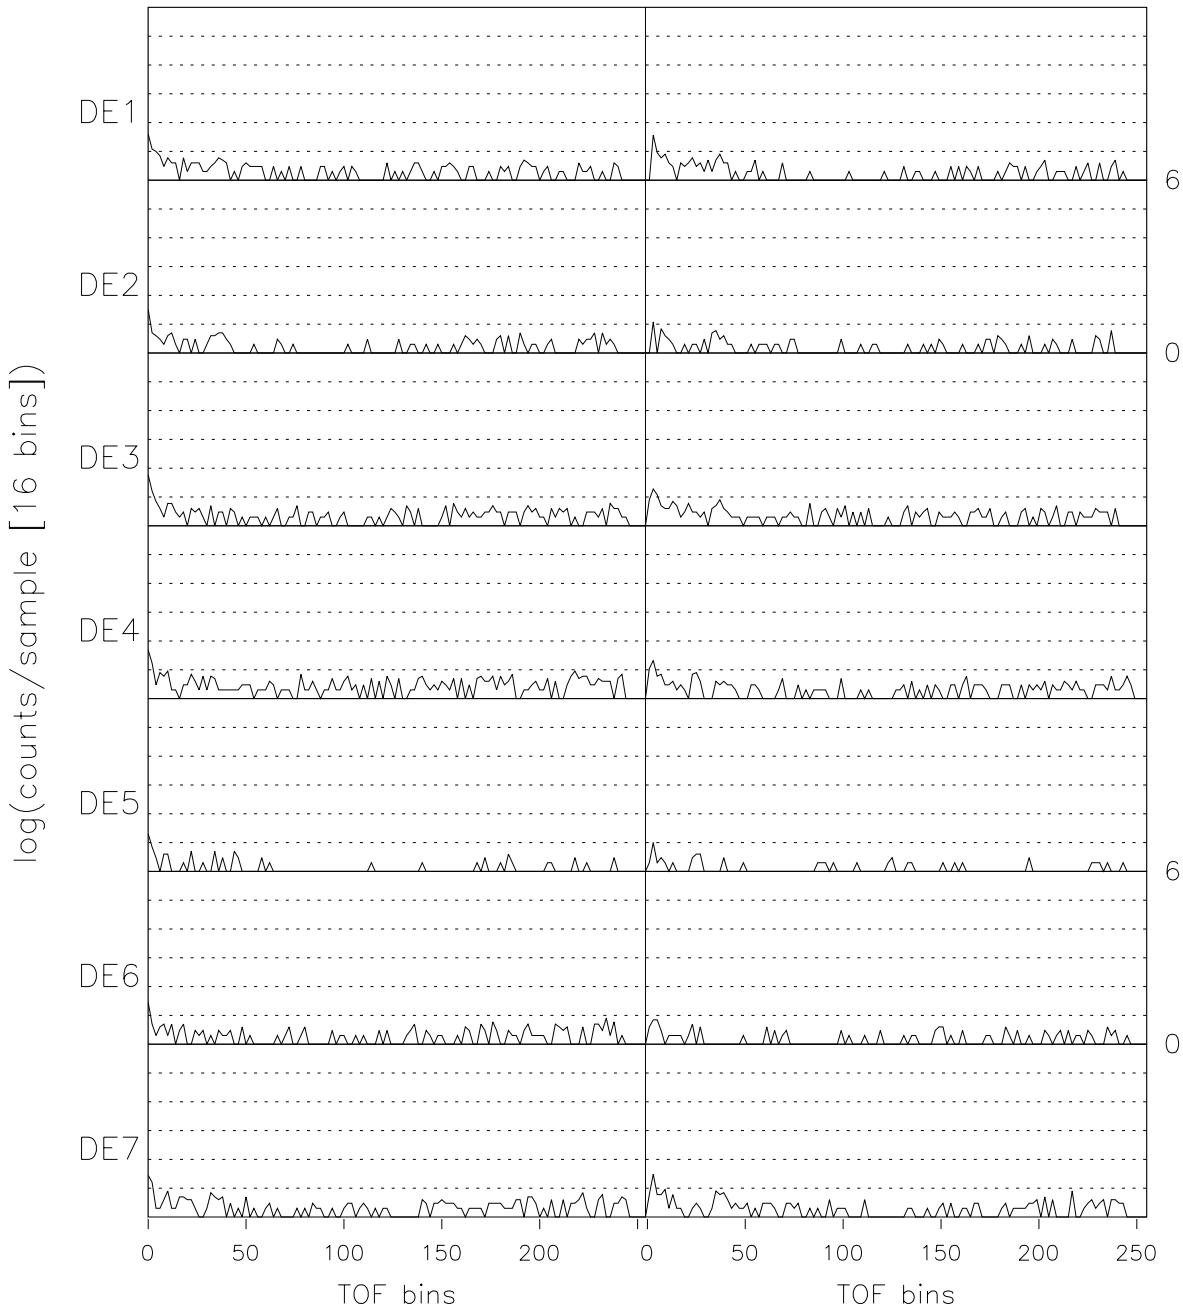

reported: 11-25-97 01:17:26 UT

reported: 11-25-97 01:20:38 UT

file: /export/data/tide/nrt/97112501.dat

-15kV TOF: -9245 v

-3.6kV MCP: -2578 v

-2.4kV MCP: -1579 v

Input Cur: 300 ma

RPA max: 236 v

Mirror max: 238 v